WIRE IDENTIFICATION	WIRE COLOUR	DESCRIPTION	CONDUCTOR SIZE
E	GREEN/YELLOW	SUPPLY EARTH	50/0.25 (2.5mm²)
L1	BLACK	MAINS SUPPLY	50/0.25 (2.5mm²)
L2	BLACK	MAINS SUPPLY	50/0.25 (2.5mm²)
L3	BLACK	MAINS SUPPLY	50/0.25 (2.5mm²)
N	BLACK	MAINS NEUTRAL	50/0.25 (2.5mm²)
⏚	GREEN/YELLOW	CABINET EARTH	30/0.25 (1.5mm²)
8	VIOLET	0V DC	16/0.2 (0.5mm²)
24	PINK	+24V DC	16/0.2 (0.5mm²)
ALL OTHER WIRES	BLACK	<3Amp	16/0.2 (0.5mm²)
		>3Amp & <16Amp	30/0.25 (1.5mm²)
		>16Amp	50/0.25 (2.5mm²)

REVISION RECORD

ISSUE	DATE	DESCRIPTION OF CHANGES	DC	SEE PAGES	AUTHORITY	DRN
A	18/06/13	FIRST RELEASE		ALL	S. SMITH	ADED
B	28/11/14	UPDATED PIN 4 NOTATION TO 270 AND PUT IN JUMP TO EASE READABILITY		2	S. SMITH	RK
C	04/02/15	WIRE IDENTIFICATION NUMBERS UPDATED FOR 210 AND 211		ALL	M.RYLEY	IL
D	20/05/15	ATCU260 Y2 BYPASS REMOVED COLOURS ADDED TO WIRES		2		LSAUN
E	24/04/18	REMOVAL OF MANUFACTURER AND ADDED PART NUMBERS		ALL	S. SMITH	VM
F	09/10/18	ADDED PINS 13, 14, 15, 16, 7 & 9, REMOVED ELEC271 & NOW ELEC062 & ELEC063 WAS RELC065		ALL	S. SMITH	VM
G	03/01/24	CHANGED TO A 3 PHASE SYSTEM		ALL	S. SMITH	SQ
H	05/09/24	RCBO ADDED. WIRE NUMBERS UPDATED TO MATCH CHAMBER		ALL	S. SMITH	SQ
I	12/06/25	RCBO CHANGED TO RCD WITH MCB PROTECTION. CABLE SIZES ADDED.		2	S. SMITH	SQ
J	18/06/26	PSYCHOMETRIC PUMP NOW 230VAC, WIRE 71 IS NOW 265		2, 3, 4	S. SMITH	MW
K	05/10/2026	16 WAY PLUG FOR UMBILICAL ELEC9951 INSTEAD OF 24 WAY		3	S. SMITH	MW

1	2	3	4	5	6	7	8	9

ascott

KEY TO MODELS COVERED

	B		F		
	C		G		J
	D		H		K
	E				L


TITLE: ACC112 - MIDI UNIT 380-440VAC 3 PHASE WITH PSYCHROMETRIC HUMIDITY

PRODUCT CODE	DRAWING NUMBER	ISSUE	PAGE	
ELES180	DRG654	K	1 OF 4	REVISION TABLE

ASCOTT ANALYTICAL EQUIPMENT LTD
UNIT 6, GERARD
LICHFIELD ROAD INDUSTRIAL ESTATE
TAMWORTH
STAFFS
B79 7UW

TEL: +44(0)1827 318040
FAX: +44(0)1827 318049
E-MAIL: info@ascott-analytical.com

DRAWN	CHECKED	DATE
MW	S SMITH	05/10/2026

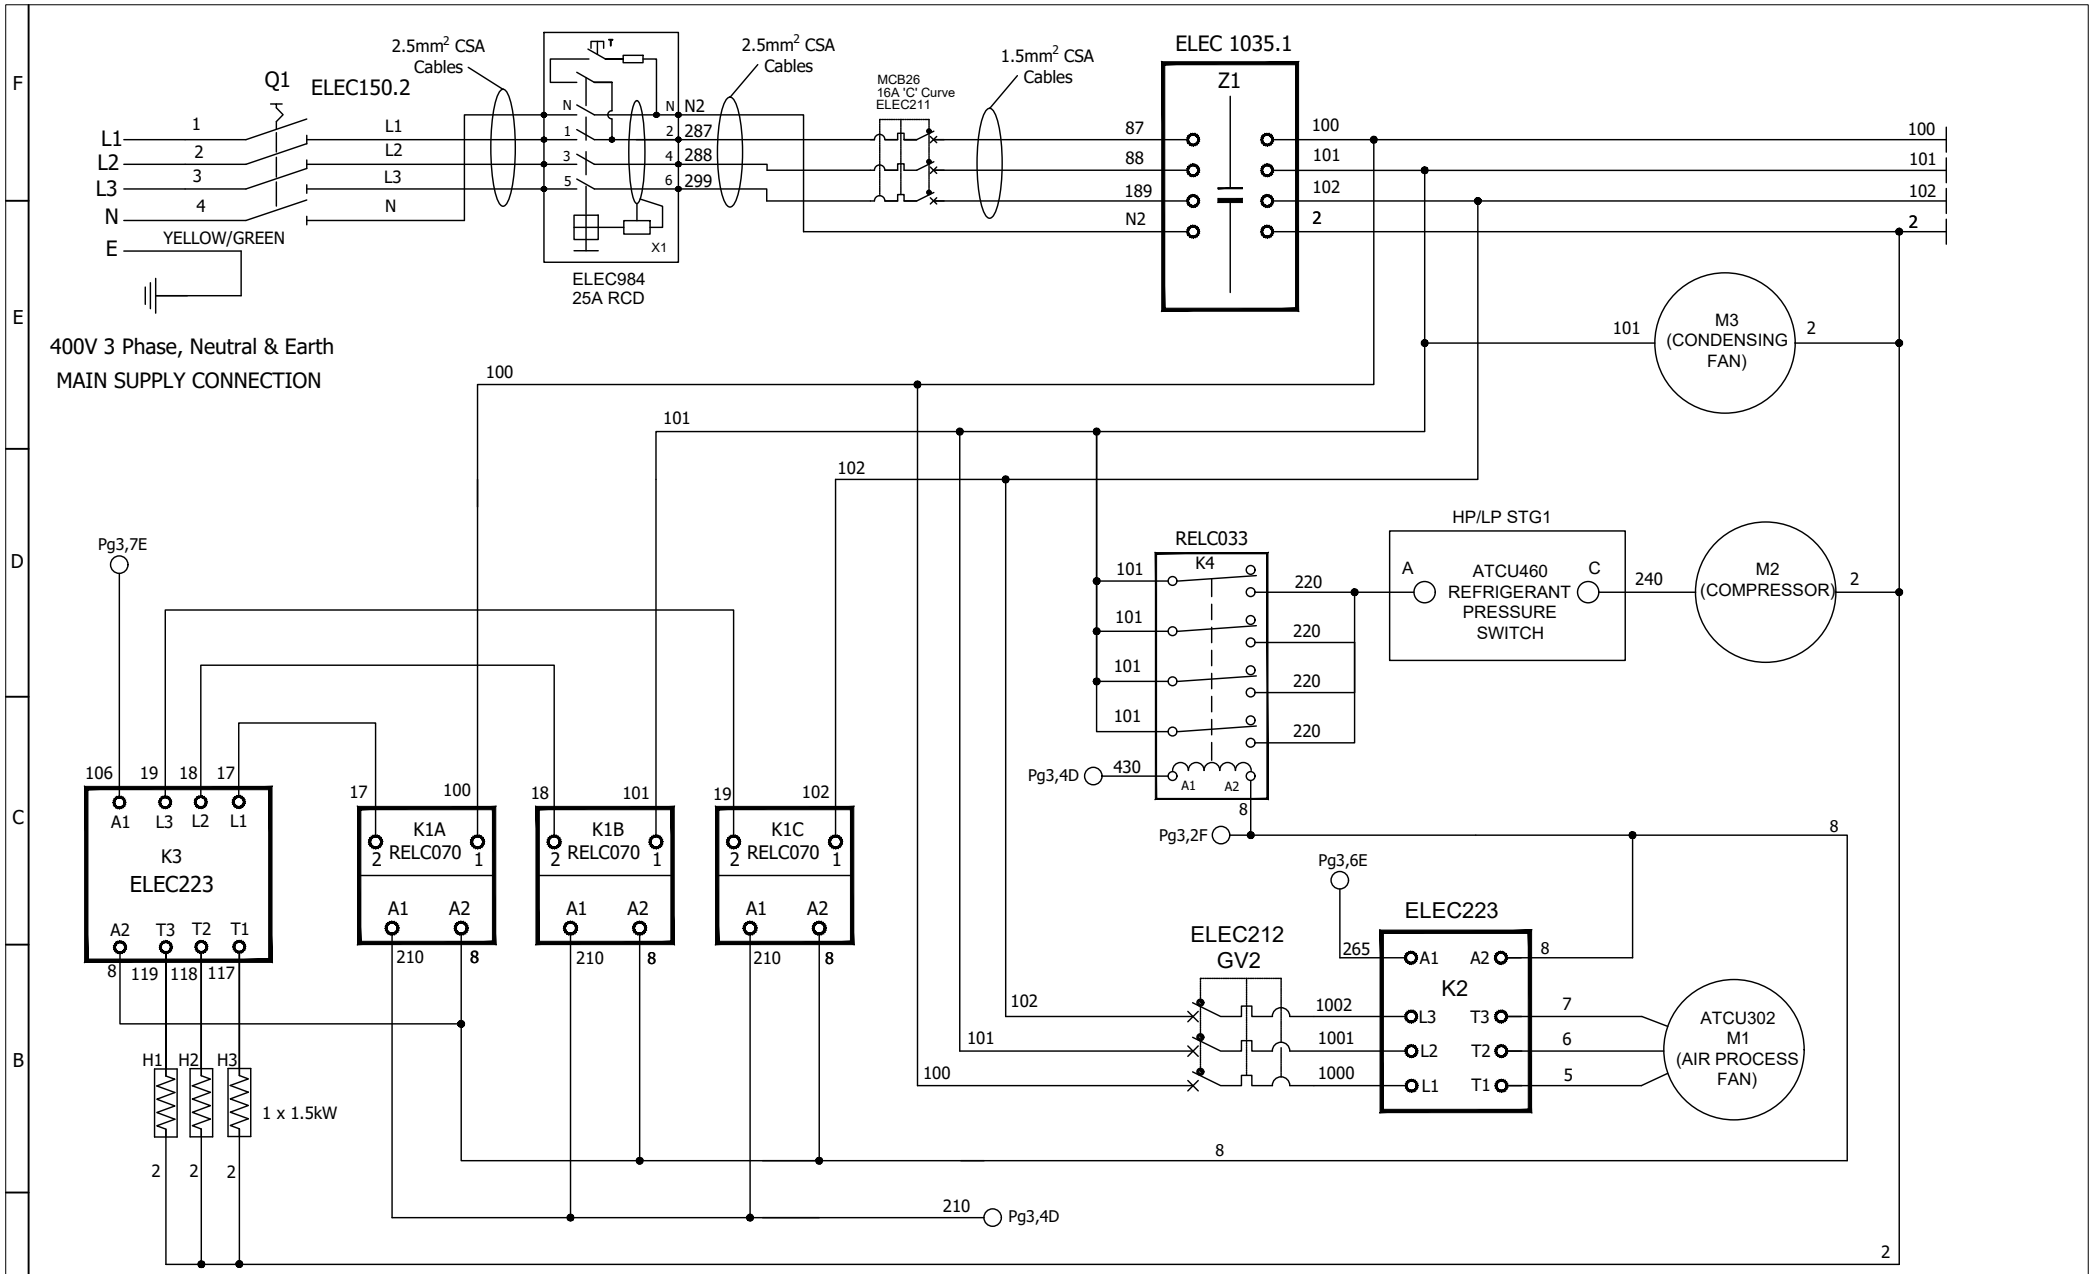

1	2	3	4	5	6	7	8	9

ascott

KEY TO MODELS COVERED

	B		F		
	C		G		J
	D		H		K
	E				L


TITLE: ACC112 - MIDI UNIT 380-440VAC 3 PHASE WITH PSYCHROMETRIC HUMIDITY

PRODUCT CODE	DRAWING NUMBER	ISSUE	PAGE	
ELES180	DRG654	K	2 OF 4	POWER MANAGEMENT

ASCOTT ANALYTICAL EQUIPMENT LTD
UNIT 6, GERARD
LICHFIELD ROAD INDUSTRIAL ESTATE
TAMWORTH
STAFFS
B79 7UW

TEL: +44(0)1827 318040
FAX: +44(0)1827 318049
E-MAIL: info@ascott-analytical.com

DRAWN	CHECKED	DATE
MW	S SMITH	05/10/2026

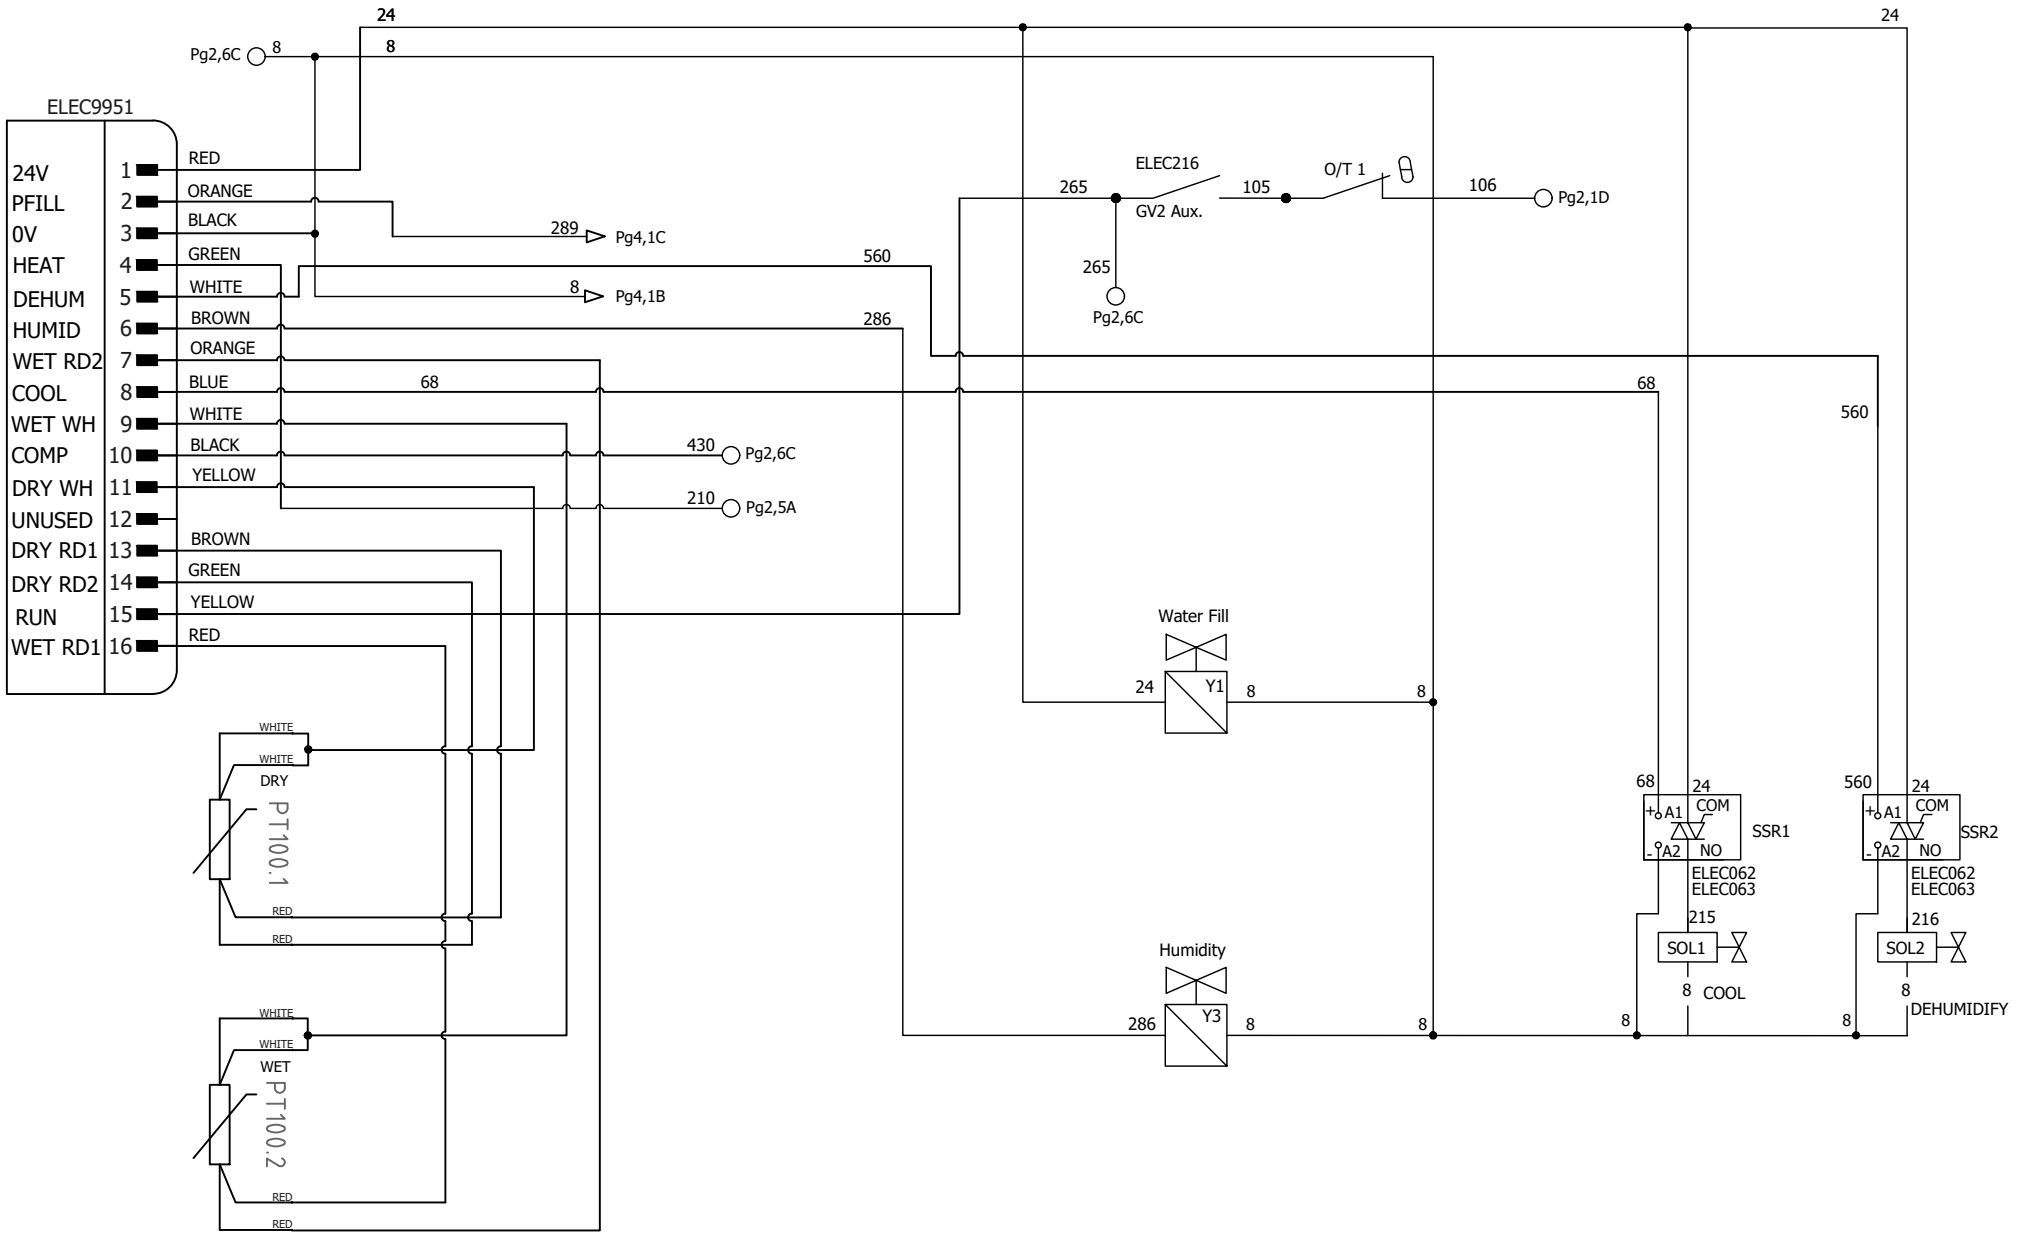

1	2	3	4	5	6	7	8	9

ascott

KEY TO MODELS COVERED

	B		F		
	C		G		J
	D		H		K
	E				L


TITLE: ACC112 - MIDI UNIT 380-440VAC 3 PHASE WITH PSYCHROMETRIC HUMIDITY

PRODUCT CODE	DRAWING NUMBER	ISSUE	PAGE	
ELES180	DRG654	K	3 OF 4	FUNCTIONS

ASCOTT ANALYTICAL EQUIPMENT LTD
UNIT 6, GERARD
LICHFIELD ROAD INDUSTRIAL ESTATE
TAMWORTH
STAFFS
B79 7UW

TEL: +44(0)1827 318040
FAX: +44(0)1827 318049
E-MAIL: info@ascott-analytical.com

DRAWN	CHECKED	DATE
MW	S SMITH	05/10/2026

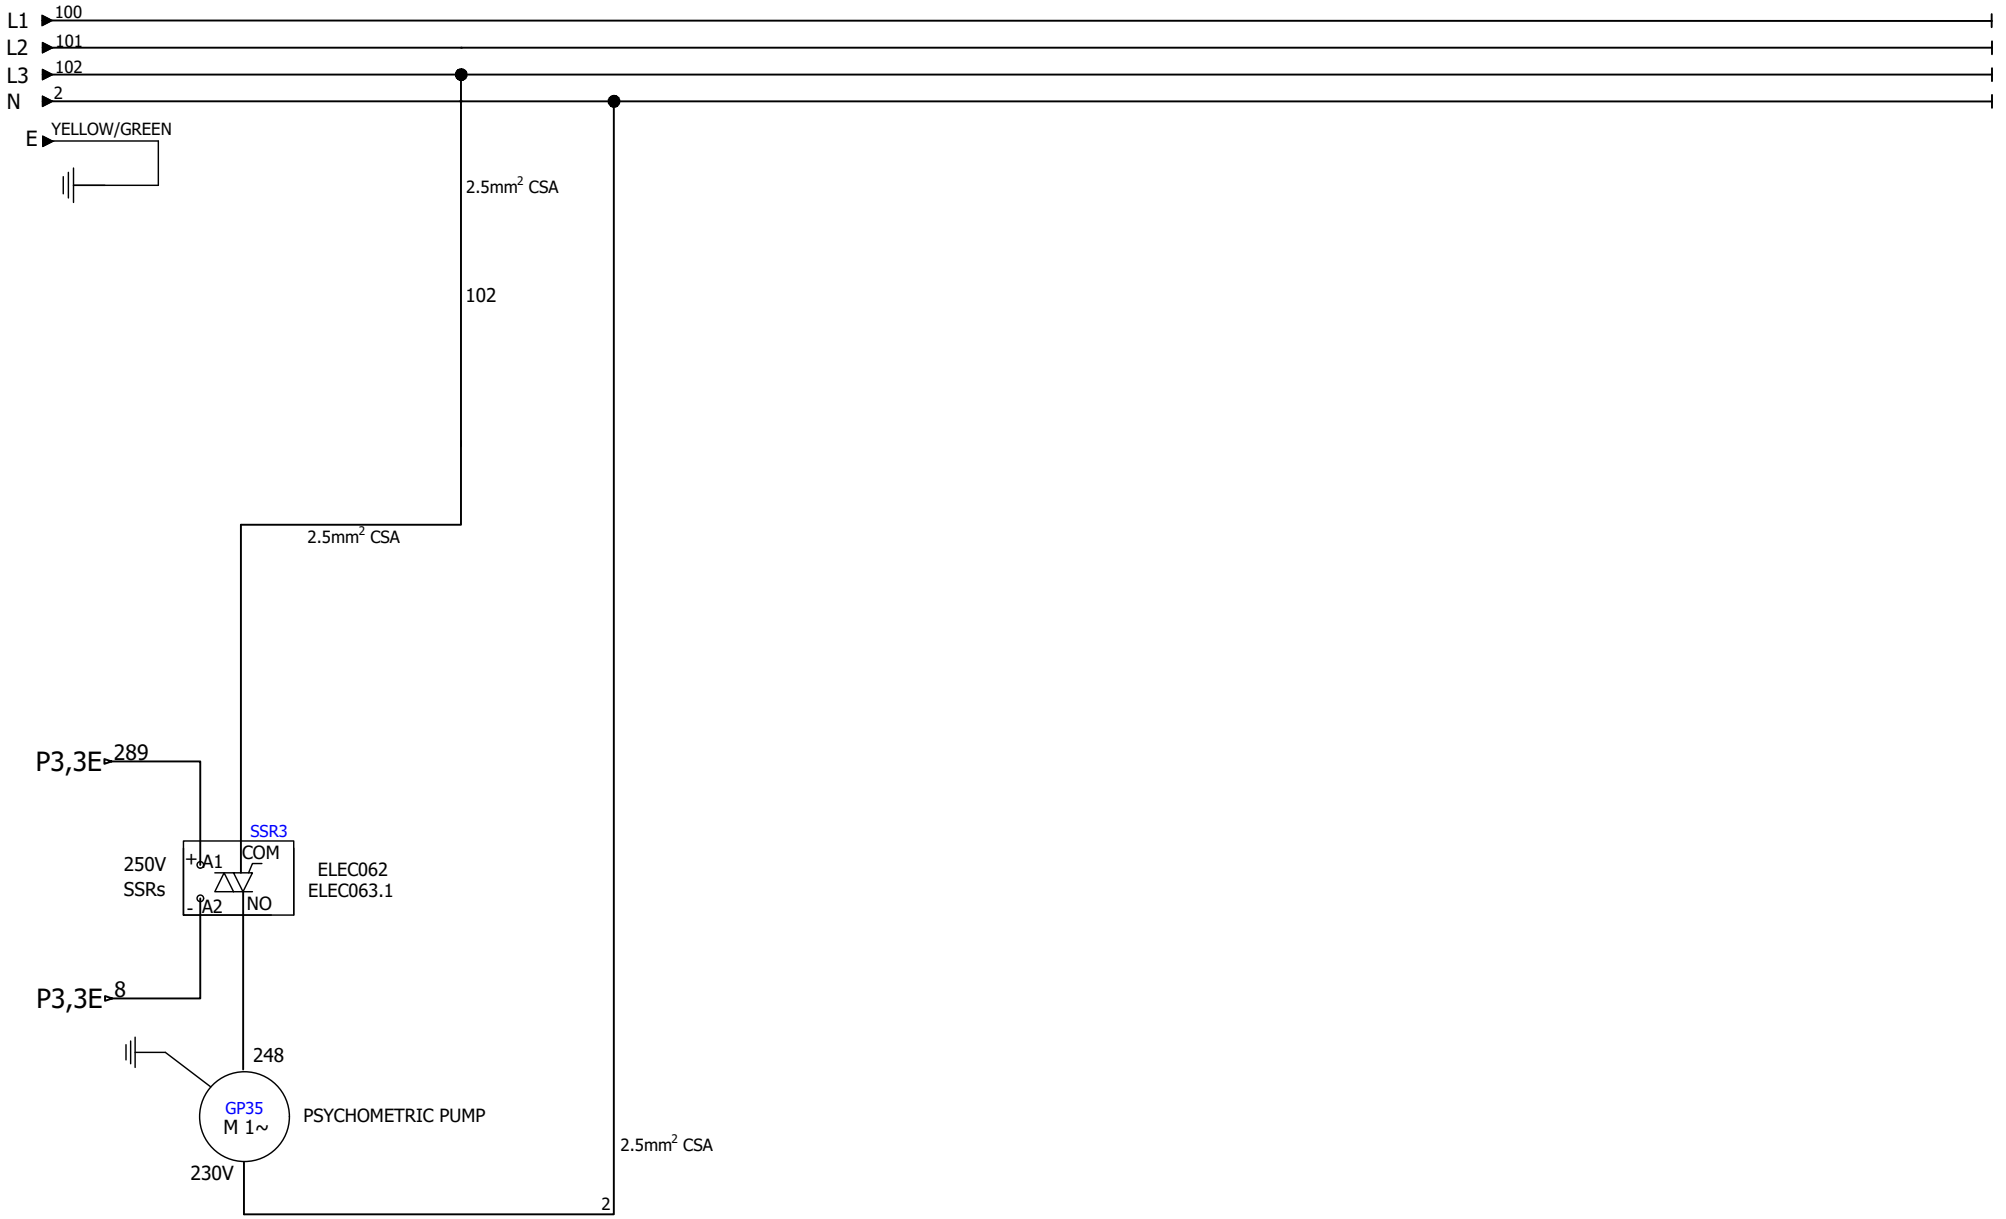

1	2	3	4	5	6	7	8	9

ascott

KEY TO MODELS COVERED

	A		E		I			
	B		F		J			
	C		G		K			
	D		H		L			

TITLE: ACC112 - MIDI UNIT 380-440VAC 3 PHASE WITH PSYCHROMETRIC HUMIDITY

PRODUCT CODE	DRAWING NUMBER	ISSUE	PAGE	NAME
ELES180	DRG654	K	4 of 4	PSYCHOMETRIC PUMP

ASCOTT ANALYTICAL EQUIPMENT LTD
UNIT 6, GERARD
LICHFIELD ROAD INDUSTRIAL ESTATE
TAMWORTH
STAFFS
B79 7UW

TEL: +44(0)1827 318040
FAX: +44(0)1827 318049
E-MAIL: info@ascott-analytical.com

DRAWN	CHECKED	DATE
MW	S SMITH	05/10/2026